


## LOWER EXTREMITY PAIN

Start treating with ~10-15 probe placements at different angles as illustrated and described below. This represents one treatment set, which may need to be repeated. Bracket the treated area with probes so that current flows *through* the area of pain. Press probes *firmly* to bare skin and apply current 10 sec. per placement. When the timer beeps, move probes quickly to a new placement and hold firmly until next beep. Repeat treatment sets as needed. Remember to rate patient's pain on a 0-10 scale before treatment and between individual treatment sets.

Stop treatment when pain is completely gone or when the improvement has reached a plateau after several treatment sets. *For optimal results, always follow the probe treatment with cranial electrotherapy stimulation (CES).*

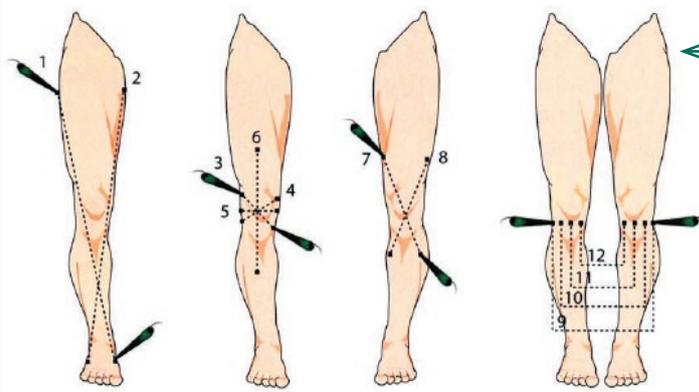


1-2. First make a large "X" by treating from the medial, superior thigh to the lateral foot, then the lateral hip to the medial foot.

3-6. Complete 40 sec. to 1 min. of smaller X's closer to and directly around the area of pain (e.g. hip, knee, ankle, foot, etc.).

7-8. Treat the *opposite* extremity (e.g. hip, knee, ankle, foot, etc.) in the same manner for 20 to 40 sec. even if there is no pain present.

9-12. Connect the two lower extremities (e.g., hip, knee, ankle, foot, etc.) by placing one probe on each in several symmetrical places encompassing the pain area for 40 sec. to 1 min.

A very rapid effective means of pain relief is to simply place the probes on the opposite extremities simultaneously in equal contralateral locations.

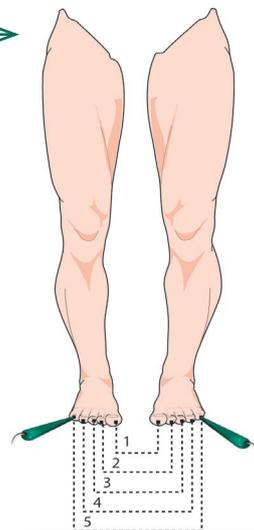

For example, for knee pain a probe is placed on each toe in succession as shown here (1-5). This will often alleviate pain within 1 min. This placement may be used for pain of the lower extremity, pelvis, hip, and low back.

**The 1-Minute Probe Treatment Protocol**

*Note: Similarly, simultaneous probe placements on the fingers will treat the upper extremity, shoulders and neck pain problems.*

### Stimulation Settings (treatment probes)

**Alpha-Stim® Model:**  
Alpha-Stim® 100

#### Treatment Mode:

Use a pair of treatment probes. Connect probes to lead wire and insert L-shaped plug from lead wire into channel ① output. Attach felt pads to probes. Wet pads thoroughly with Alpha Conducting Solution™. Reapply solution as needed during treatment.

#### Frequency:

Set the frequency slider switch for channel ① to 0.5Hz (far left).

#### Current Intensity:

Turn dial for channel ① to "6" (600µA) or to highest comfortable level.

#### Timer:

Set timer slider switch to "probe" (far right).

## References

Alpha-Stim® 100 Owner's Manual (2002). Electromedical Products International, Inc.

Kirsch, D. L. (2006). Microcurrent electrical therapy (MET): A tutorial. *Practical Pain Management* 6(7):59-64.

Kirsch, D. L. (2002). A practical protocol for electromedical treatment of pain. Chapter 61 (pp. 759-776) In *Pain Management: A Practical Guide for Clinicians* Weiner, R (ed.) CRC Press, Boca Raton, Florida.

The information provided in this poster is not a substitute for the Owner's Manual. Read the Prescribing Information in the Owner's Manual for Contraindications, Precautions and Adverse Effects associated with the use of Alpha-Stim®. Copyright 2007 Electromedical Products International, Inc. ALL RIGHTS RESERVED. Alpha-Stim® is registered in the US Patent and Trademark Office and worldwide.

